

FIG. 1A

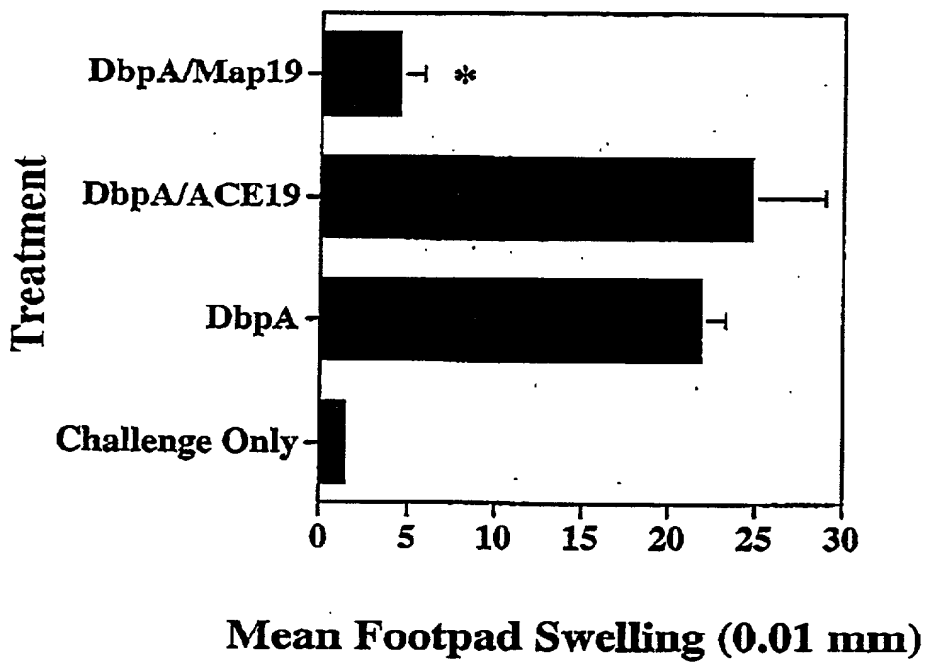


FIG. 1B

**Treatment**


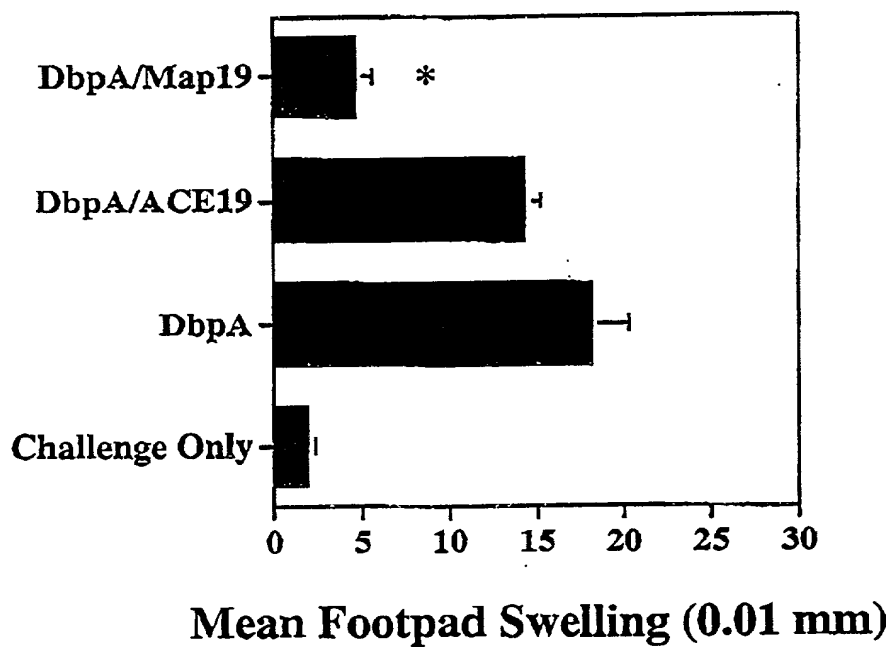


FIG 1 C

# Treatment

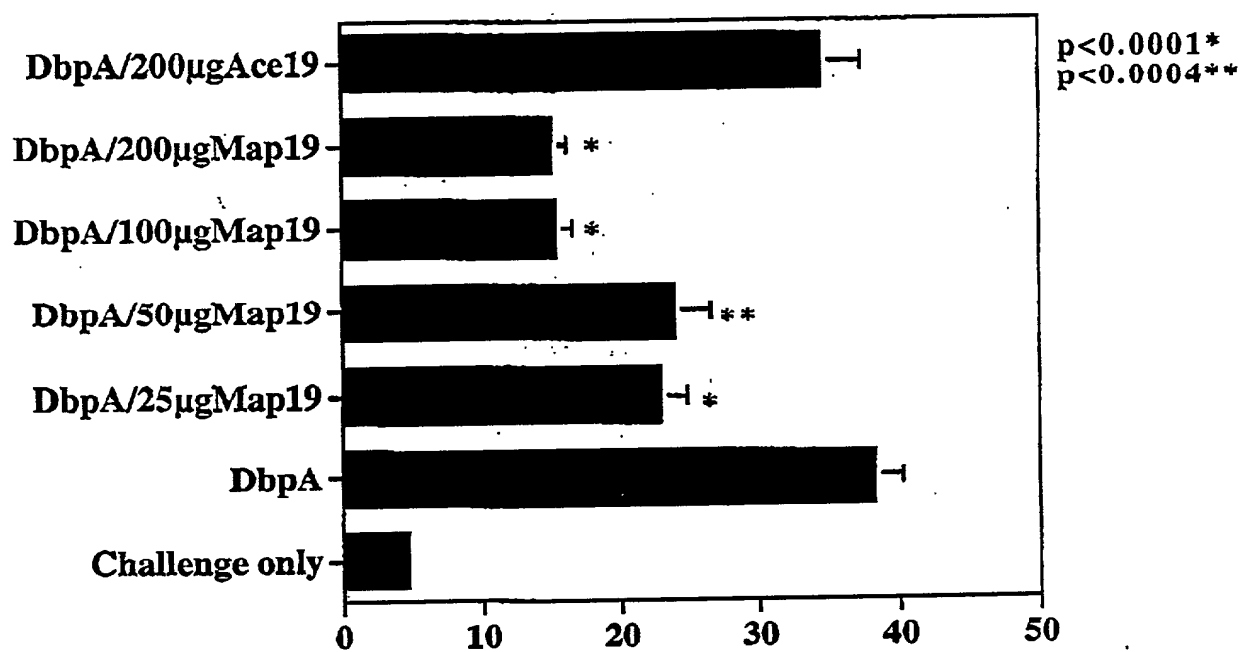

Mean Footpad Swelling (0.01mm)

FIG. 2

Effect of Treatment

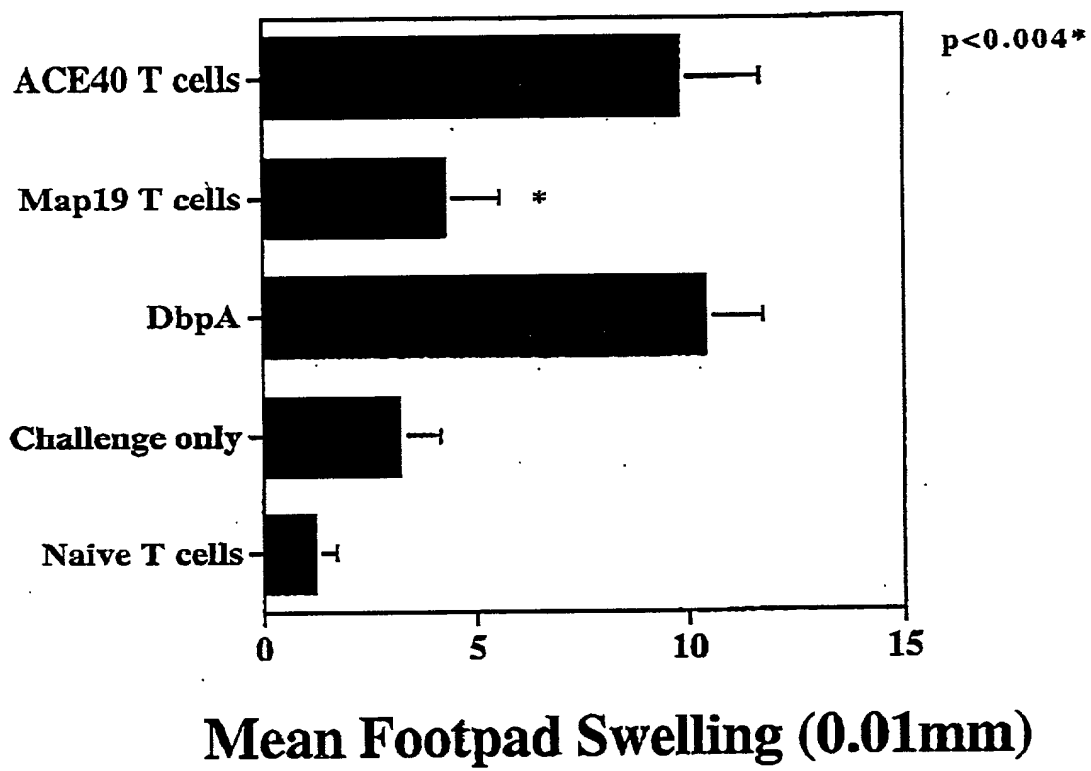


FIG. 3

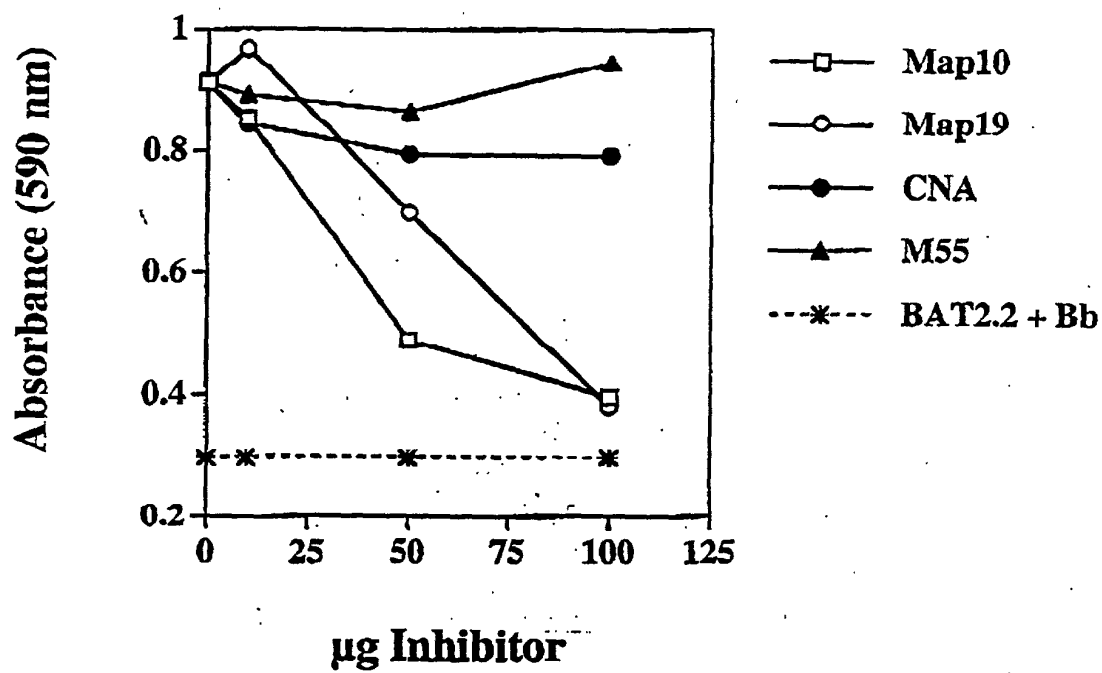


FIG. 4

